


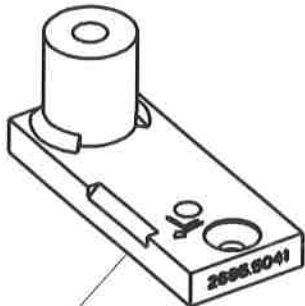
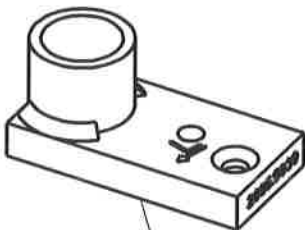
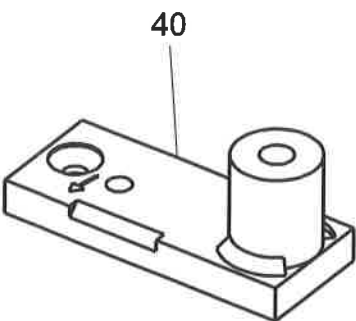
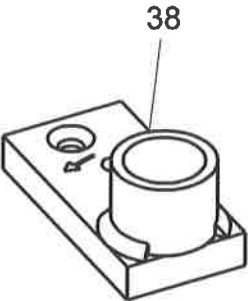


DOCUMENT  
PROVISOIRE

| REP         | REFERENCE          | MASSE | NB | CT |
|-------------|--------------------|-------|----|----|
| 37          | 2695.5037          | 1,60  | 2  |    |
| 38          | 2695.5038          | 0,61  | 1  |    |
| 39          | 2695.5039          | 0,61  | 1  |    |
| 40          | 2695.5040          | 0,91  | 1  |    |
| 41          | 2695.5041          | 0,91  | 1  |    |
| M12x1,50-70 | 7112X07043         | 0,08  | 2  |    |
| E           | 106                | 0,53  | 1  |    |
| MRI.F.01    | MRI.F.01           | 0,04  | 1  |    |
|             | BOUCHON11          |       | 4  |    |
|             | 2695.5A02-AC       |       | 2  |    |
|             | 2695.5A02-EMB-A4   |       | 1  |    |
|             | 2695.5A02-L11-A4   |       | 1  |    |
|             | 2695.5A02-CTR      |       | 1  |    |
|             | INSTRUCTION-RVA4-1 |       | 1  |    |

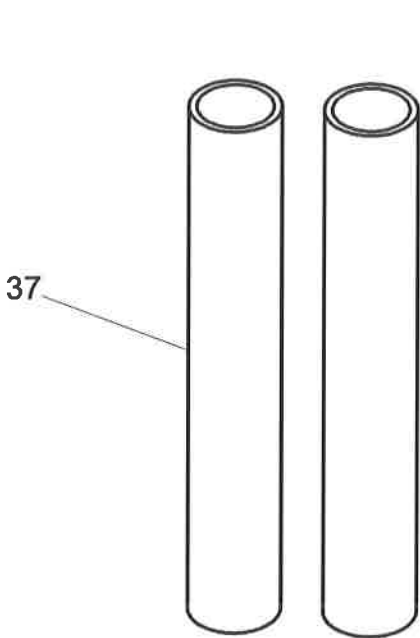

M12x1,50-70

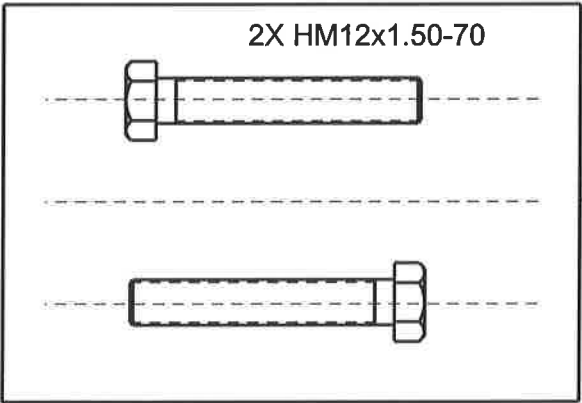

MRI.F.01

